FASTCheck15®
In-Office Water Test Strip

Understanding Your FASTCheck15® Test

Faint test lines indicate a bacterial count exceeding 500 CFU/mL and should be interpreted as a failed result.

Negative for Bacteria

1 (C) Line Present = PASS = below 500 CFU/mL




PASS

Positive for Bacteria

2 (T & C) Lines Present* = FAIL = 500 CFU/mL or above

*No matter how faint the T line is.

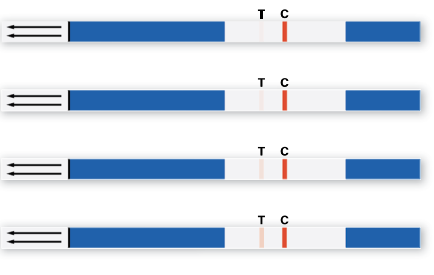

FAIL

FAIL

FAIL


FAIL

The presence of **both** a **Control** line **(C)** and a **Test** line **(T)** indicates a failed waterline test result.

T = Test
C = Control

If no Control line appears following the testing instructions, the test is invalid.

Repeat testing instructions with a new test kit.

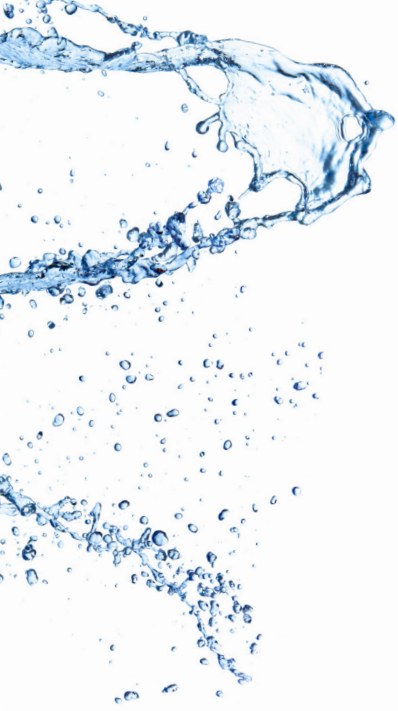

FASTCheck15®
In-Office Water Test Strip

FASTCheck15®

- Faster, easier, more affordable than paddles.
- A simple Pass/Fail result in 15 minutes.
- Regular monitoring of water to ensure compliance to the EPA Drinking Water Standards of ≤500 CFU/mL.
- Ensures patient safety and compliance.
- Validates Dental Unit Waterline Management protocols are successful.

Questions?

A Sterisil® Water Safety Specialist is here to support.

Call: 877-207-1551, Option 1 *or*
Email: SterisilSupport@Solmetex.com

STERISIL®

FASTCheck15® Resources

- Instructions For Use Video
- Testing Log
- Access My Solution Center Portal

STL-MKT-COL-473 Rev1.0